



Gas



Liquid &amp; Slurry



Solid &amp; Powder



Steam &amp; Water

# SENTRY MLG SAMPLER

## Low Emission Samplers

### MANUAL SAMPLING

The Sentry® MLG manual low emission sampler is ideal for sampling liquified petroleum gas (LPG) and other two-phase liquids—gases that are pressurized, stored and transported in their liquid phase—with high vapor pressures.

#### MODEL

MLG

#### BENEFITS

The Sentry MLG sampler incorporates a number of features to provide for safe, simple and representative sampling. The six-port tandem valve simplifies sampling by replacing multiple valve operations with just one ergonomically-designed valve. The sampler action is repeatable, so the sample is always as representative as possible.

By using an expansion vessel to reduce sample cylinder volume after the sample is captured, both safety (outage space for transport of the cylinder assembly) and representative sampling are assured for the most accurate data analysis results.

Modes of operation include:

**Off (insert cylinder):** Switching valve handle is in off position, blocking both side ports on both three-way valves on switching valve. There is no flow through the sampler.

**Sample:** Switching valve handle is turned to sample position; sample flows through sampler and connected sample cylinder, essentially a purging/filling process.

**Expansion Mode:** Used for opening the expansion cylinder to give the necessary outage in the main sample cylinder. Needs to be used before Isolate Mode.

**Isolate:** Sample is isolated in cylinder by closing cylinder valves. Outlet cylinder valve (bottom) must be closed first if sample needs to be maintained at system pressure.

**Vent:** Switching valve handle is turned to vent/depressurize position and all sample gases in the lines on either side of the sample cylinder are vented to a low pressure flare/vent header or local vapor recovery device.

**Off (remove cylinder):** Switching valve handle is turned to off position, blocking both side ports on both three-way valves on switching valve. As sampler lines are vented, disconnecting the cylinder can be done safely.

#### FEATURES

- Allows for flushing of sample panel and cylinder to increase sample accuracy without discharge to the atmosphere or wasting product
- Ergonomic design reduces turning torque and eliminates repetitive wrist action
- Six-port/multi-function tandem valve simplifies operation and reduces valve maintenance
- Variety of configurations to meet any gas sampling need
- Connection sizes from 1/4 to 1/2-inch (8 to 15 mm), including compression, socket weld, flanged or NPT
- Options include sample cooler, in-line filter, check valves, carbon canister, nitrogen purge, flow indicator, cylinder relief valve, rupture disc, pipe stand, heater and enclosures; valve package for applications without process return





Sample. Monitor. Measure.



# SENTRY

Any Application. Anywhere.

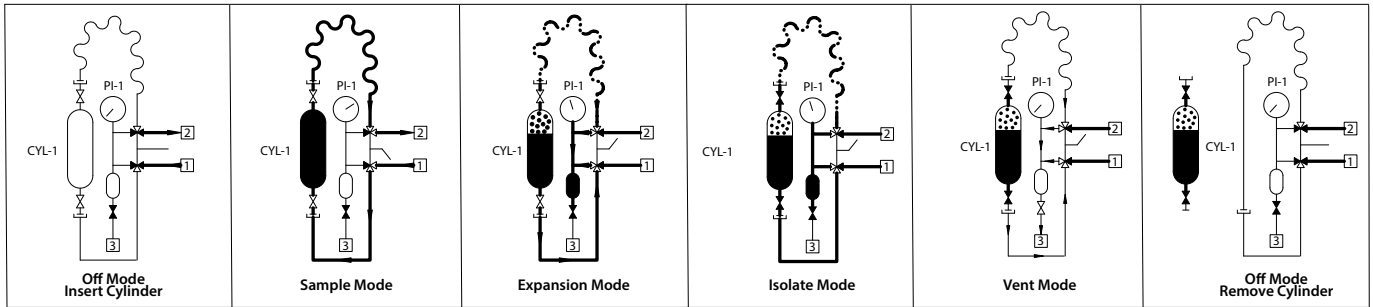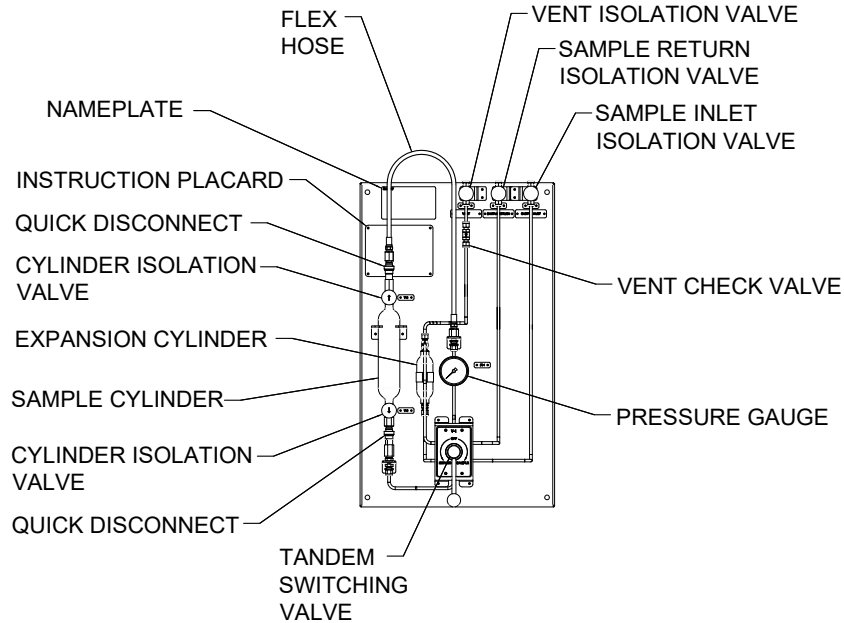

## SPECIFICATIONS

<b>materials</b>	304 stainless steel backplate; 316 or 304 stainless steel cylinders
<b>wetted materials</b>	316 stainless steel, PTFE, Viton®, Kalrez®
<b>standard pressure rating</b>	1800 psi at 100°F (125 bar at 38°C)
<b>standard temperature rating</b>	300°F at 1230 psi (149°C at 85 bar); higher temperatures available

[sentry-equip.com](http://sentry-equip.com)

966 Blue Ribbon Circle North, Oconomowoc, WI 53066 U.S.A. | +1-262-567-7256 | sales@sentry-equip.com

© 2016 Sentry Equipment Corp. All rights reserved. Sentry is a registered trademark of Sentry Equipment Corp. Viton is a registered trademark of The Chemours Company. Kalrez is a registered trademark of E.I. du Pont de Nemours and Company. It is solely the responsibility of end users, through their own testing and analysis, to select products and materials suitable for their specific application requirements, ensure they are properly installed, safely applied and properly maintained, and to limit their use to their intended purpose. Improper selection, installation or use may result in personal injury or property damage.

S-GA-SPS-00184-4 7-23



COMPANY WITH  
QUALITY SYSTEM  
CERTIFIED BY DNV GL  
= ISO 9001 =